



Tapered Screw-Vent[®] Implant System






Table of Contents

Implants	4
Trabecular Metal Implants (TM)	4
Tapered Screw-Vent Implants (TSV)	4
Healing Collars	6
Healing Collar Selection Guidelines	6
Tapered Screw-Vent (TSV) BellaTek® Encode® Healing Abutments	6
Healing Collars	6
Prosthetics	7
Impression Transfer	7
Provisional Restorations	8
Cement-Retained Restorations	9
Custom Restorations	12
Screw-Retained Restorations	14
Components for Screw-Retained Restorations	15
Overdenture Attachments	17
Prosthetic Tools	19
Instrument Kit System	22
Instrument Kit System Overview	22
Tapered Screw-Vent Surgical Kit (TSVKIT)	24
Guided Surgery Instrumentation	26
Dríva™ Surgical Drills	27
Instrumentation	28
Drill Stop Kit	30

Surgical Cover Screws





Included with Implant.

Implant Platform		
 3.5 mmD	 4.5 mmD	 5.7 mmD
TSC	TSCW	TSC5



TM Dental Implant, MTX® Surface, Fully Textured with Microgrooves





Includes Fixture Mount/Transfer and Cover Screw.

Implant Diameter	Implant Platform	Internal Hex Connection	Implant Length			
			10 mmL	11.5 mmL	13 mmL	16 mmL
3.7 mmD	 3.5 mmD	2.5 mmD	TMTB10	TMTB11	TMTB13	TMTB16
4.1 mmD	 3.5 mmD*	2.5 mmD	TMT4B10	TMT4B11	TMT4B13	—
4.7 mmD	 4.5 mmD	2.5 mmD	TMTWB10	TMTWB11	TMTWB13	—
6.0 mmD	 5.7 mmD	3.0 mmD	TMT6B10	TMT6B11	TMT6B13	—



TM Dental Implants with 0.5 mm Machined Collar, MTX Surface, and Microgrooves





Includes Fixture Mount/Transfer and Cover Screw.

Implant Diameter	Implant Platform	Internal Hex Connection	Implant Length			
			10 mmL	11.5 mmL	13 mmL	16 mmL
3.7 mmD	 3.5 mmD	2.5 mmD	TMMB10	TMMB11	TMMB13	TMMB16
4.1 mmD	 3.5 mmD*	2.5 mmD	TMM4B10	TMM4B11	TMM4B13	—
4.7 mmD	 4.5 mmD	2.5 mmD	TMMWB10	TMMWB11	TMMWB13	—
6.0 mmD	 5.7 mmD	3.0 mmD	TMM6B10	TMM6B11	TMM6B13	—



TSV Implants with Full MTX Surface Texturing and Microgrooves





Includes Fixture Mount/Transfer and Cover Screw.

Implant Diameter	Implant Platform	Internal Hex Connection	Implant Length				
			8.0 mmL	10 mmL	11.5 mmL	13 mmL	16 mmL
3.7 mmD	 3.5 mmD	2.5 mmD	TSVTB8	TSVTB10	TSVTB11	TSVTB13	TSVTB16
4.1 mmD	 3.5 mmD*	2.5 mmD	TSVT4B8	TSVT4B10	TSVT4B11	TSVT4B13	TSVT4B16
4.7 mmD	 4.5 mmD	2.5 mmD	TSVTWB8	TSVTWB10	TSVTWB11	TSVTWB13	TSVTWB16
6.0 mmD	 5.7 mmD	3.0 mmD	TSVT6B8	TSVT6B10	TSVT6B11	TSVT6B13	TSVT6B16



TSV Implants with 0.5 mm Machined Collar, MTX Surface, and Microgrooves

Includes Fixture Mount/Transfer and Cover Screw/

Implant Diameter	Implant Platform	Internal Hex Connection	Implant Length				
			8.0 mmL	10 mmL	11.5 mmL	13 mmL	16 mmL
3.7 mmD	 3.5 mmD	2.5 mmD	TSVMB8	TSVMB10	TSVMB11	TSVMB13	TSVMB16
4.1 mmD	 3.5 mmD*	2.5 mmD	TSVM4B8	TSVM4B10	TSVM4B11	TSVM4B13	TSVM4B16
4.7 mmD	 4.5 mmD	2.5 mmD	TSVMWB8	TSVMWB10	TSVMWB11	TSVMWB13	TSVMWB16
6.0 mmD	 5.7 mmD	3.0 mmD	TSVM6B8	TSVM6B10	TSVM6B11	TSVM6B13	TSVM6B16



TSV Implants with MTX Surface

Includes Fixture Mount/Transfer and Cover Screw.

Implant Diameter	Implant Platform	Internal Hex Connection	Implant Length				
			8.0 mmL	10 mmL	11.5 mmL	13 mmL	16 mmL
3.7 mmD	● 3.5 mmD	2.5 mmD	TSVB8	TSVB10	TSVB11	TSVB13	TSVB16
4.1 mmD	● 3.5 mmD*	2.5 mmD	TSV4B8	TSV4B10	TSV4B11	TSV4B13	TSV4B16
4.7 mmD	● 4.5 mmD	2.5 mmD	TSVWB8	TSVWB10	TSVWB11	TSVWB13	TSVWB16
6.0 mmD	● 5.7 mmD	3.0 mmD	TSV6B8	TSV6B10	TSV6B11	TSV6B13	TSV6B16



TSV Implants with MTX Textured Collar, Microgrooves, and MP-1® HA Dual Transition Selective Surface

Includes Fixture Mount/Transfer and Cover Screw.

Implant Diameter	Implant Platform	Internal Hex Connection	Implant Length				
			8.0 mmL	10 mmL	11.5 mmL	13 mmL	16 mmL
3.7 mmD	● 3.5 mmD	2.5 mmD	TSVTH8	TSVTH10	TSVTH11	TSVTH13	TSVTH16
4.1 mmD	● 3.5 mmD*	2.5 mmD	TSVT4H8	TSVT4H10	TSVT4H11	TSVT4H13	TSVT4H16
4.7 mmD	● 4.5 mmD	2.5 mmD	TSVTWH8	TSVTWH10	TSVTWH11	TSVTWH13	TSVTWH16
6.0 mmD	● 5.7 mmD	3.0 mmD	TSVT6H8	TSVT6H10	TSVT6H11	TSVT6H13	TSVT6H16



TSV Implants with 0.5 mm Machined Collar, Microgrooves, and MP-1 HA Dual Transition Selective Surface

Includes Fixture Mount/Transfer and Cover Screw.

Implant Diameter	Implant Platform	Internal Hex Connection	Implant Length				
			8.0 mmL	10 mmL	11.5 mmL	13 mmL	16 mmL
3.7 mmD	● 3.5 mmD	2.5 mmD	TSVMH8	TSVMH10	TSVMH11	TSVMH13	TSVMH16
4.1 mmD	● 3.5 mmD*	2.5 mmD	TSVM4H8	TSVM4H10	TSVM4H11	TSVM4H13	TSVM4H16
4.7 mmD	● 4.5 mmD	2.5 mmD	TSVMWH8	TSVMWH10	TSVMWH11	TSVMWH13	TSVMWH16
6.0 mmD	● 5.7 mmD	3.0 mmD	TSVM6H8	TSVM6H10	TSVM6H11	TSVM6H13	TSVM6H16



TSV Implants with MP-1 Dual Transition Selective Surface

Includes Fixture Mount/Transfer and Cover Screw.

Implant Diameter	Implant Platform	Internal Hex Connection	Implant Length				
			8.0 mmL	10 mmL	11.5 mmL	13 mmL	16 mmL
3.7 mmD	● 3.5 mmD	2.5 mmD	TSVH8	TSVH10	TSVH11	TSVH13	TSVH16
4.1 mmD	● 3.5 mmD*	2.5 mmD	TSV4H8	TSV4H10	TSV4H11	TSV4H13	TSV4H16
4.7 mmD	● 4.5 mmD	2.5 mmD	TSVWH8	TSVWH10	TSVWH11	TSVWH13	TSVWH16
6.0 mmD	● 5.7 mmD	3.0 mmD	TSV6H8	TSV6H10	TSV6H11	TSV6H13	TSV6H16



* While the implant platform color code for the 4.1 mmD TSV Implant is green, the implant surgical sequence is color-coded white on the surgical kit surface.

Healing Collars

Healing Collar Selection Guidelines

Selecting a Healing Collar:

- Determine the size of the implant platform
- Select the emergence profile that best suits the site being restored. The profile should match the transfer and abutment to be used
- Select the cuff height so that the top of the component protrudes slightly above the surrounding tissue. The options are 3.0 mm, 5.0 mm, or 7.0 mm

HC3/TEHA3 = 3.5 mmD (Implant Platform) Healing Collar


HC4/TEHA4 = 4.5 mmD (Implant Platform) Healing Collar

HC5/TEHA5 = 5.7 mmD (Implant Platform) Healing Collar

Example:

HC343 = 3.5 mmD (Implant Platform) Healing Collar, 4.5 mmD Emergence Profile, 3.0 mm Cuff Height (second digit equals profile, third digit equals height)

TEHA3383 = 3.5 mmD (Implant Platform) Healing Collar, 3.8 mmD Emergence Profile, 3.0 mm Cuff Height (middle two digits equals profile, last digit equals height)

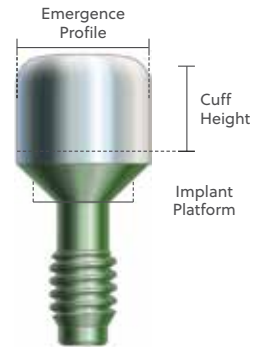


TSV Connection Implants

Platform Diameter	Emergence Profile	Height		
		3	5	7
● 3.5 mmD	3.8	TEEHA333	TEEHA335	TEEHA337
	5.0	TEEHA353	TEEHA355	TEEHA357
	6.5	TEEHA363	TEEHA365	TEEHA367
● 4.5 mmD	4.5	TEEHA443	TEEHA445	TEEHA447
	5.5	TEEHA453	TEEHA455	TEEHA457
	6.5	TEEHA463	TEEHA465	TEEHA467
	7.5	TEEHA473	TEEHA475	TEEHA477
● 5.7 mmD	5.7	TEEHA553	TEEHA555	-
	6.8	TEEHA563	TEEHA565	-
	7.5	TEEHA573	TEEHA575	-



Healing Collars

Platform Diameter	Emergence Profile	Height		
		3	5	7
● 3.5 mmD	3.5 mmD (No Flare)	HC333	HC335	—
	4.5 mmD	HC343	HC345	HC347
	5.5 mmD	HC353	HC355	—
● 4.5 mmD	4.5 mmD (No Flare)	HC443	HC445	—
	5.5 mmD	HC453	HC455	HC457
	6.5 mmD	HC463	HC465	—
	6.5 mmD	HC563	HC565	—
● 5.7 mmD	5.7	TEEHA553	TEEHA555	-

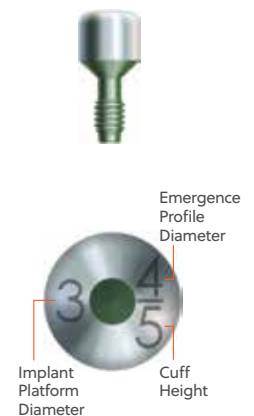

Prosthetics


Impression Transfers

Multi-Purpose Fixture Mount/Transfer

TSV and TM Implants are packaged with a Fixture Mount/Transfer that serves multiple functions:

Implant Placement

The Fixture Mount is used as a means to deliver the implant to the surgical site and provides convenient color-coded identification that matches the implant analogs.

 Green	3.5 mmD Platform
 Purple	4.5 mmD Platform
 Yellow	5.7 mmD Platform

Implant-Level Transfer

The Fixture Mount then functions as a transfer that is conveniently pre-attached to the implant. Surgeons can take an immediate index or impression to complete the transfer, or restoring doctors can use it after the healing period.




Preparable Temporary Abutment

The Fixture Mount may also be prepared to function as a temporary abutment while the final restoration is being fabricated. Note: The Fixture Mount is not indicated as a final abutment as it does not achieve the friction-fit connection with the implant.



Fixture Mount/Transfers




Includes a Retaining Screw (URS2). Can be used as a Preparable Temporary Abutment.

Implant Platform	Emergence Profile	Item No.
 3.5 mmD	4.5 mmD	FMT3
 4.5 mmD	5.5 mmD	FMT4
 5.7 mmD	6.5 mmD	FMT5
Replacement Retaining Screw	—	URS2



Indirect Transfers (Closed-Tray Procedure)

Color-coded by implant platform. Includes a Retaining Screw.

Implant Platform	Emergence Profile			
	3.5 mmD	4.5 mmD	5.5 mmD	6.5 mmD
 3.5 mmD	HLT3/3	HLT3/4	HLT3/5	—
 4.5 mmD	—	HLT4/4	HLT4/5	HLT4/6
 5.7 mmD	—	—	—	HLT5/6
3.0 mm Extension Screw for Indirect Transfer	HLTE	HLTE	HLTE	HLTE
Replacement Retaining Screw	HLTS2	HLTS2	HLTS2	HLTS2



Direct Transfers (Open-Tray Procedure)

Color-coded by implant platform. Includes a Retaining Screw (DHTS).

Implant Platform	Emergence Profile			
	3.5 mmD	4.5 mmD	5.5 mmD	6.5 mmD
● 3.5 mmD	DHT3/3	DHT3/4	DHT3/5	—
● 4.5 mmD	—	DHT4/4	DHT4/5	DHT4/6
Replacement Retaining Screw	DHTS	DHTS	DHTS	DHTS



Note: Direct Transfers for open-tray procedures are not available for 6.0 mmD implants with 5.7 mmD platforms (please see Indirect Transfers on previous page).

Titanium Implant Analogs for Stone Models

Color-coded by implant platform.

Implant Platform	Item No.
● 3.5 mmD	IA3
● 4.5 mmD	IA4
● 5.7 mmD	IA5



Digital Lab Analogs for 3D Printed Models

Color-coded by implant platform.

Implant Platform	Item No.
● 3.5 mmD	ILATSV35
● 4.5 mmD	ILATSV45
● 5.7 mmD	ILATSV57



Provisional Restorations

Plastic Temporary Abutments, Straight

Includes Retaining Screw and Processing Screw (DHTS2).

Implant Platform	Emergence Profile	Cuff Height	
		1.0 mm	4.0 mm
● 3.5 mmD	4.5 mmD	PT341S	PT344S
● 4.5 mmD	5.5 mmD	PT451S	PT454S
● 5.7 mmD	6.5 mmD	PT561S	PT564S
Replacement Retaining Screw, Long		DHTS2	DHTS2



Plastic Temporary Abutments, Angled, 17°

Includes Retaining Screw and Processing Screw (DHTS2).




Implant Platform	Emergence Profile	Cuff Height	
		1.0 mm	4.0 mm
● 3.5 mmD	4.5 mmD	PT341A	PT344A
● 4.5 mmD	5.5 mmD	PT451A	PT454A
Replacement Retaining Screw, Long		DHTS2	DHTS2



Cement-Retained Restorations

Color Coding Chart: Emergence Profile on Hex-Lock® Contour and Short Restorative Abutments/Components









Colors correspond to the abutment emergence profile on Hex-Lock Contour and Short Abutments and related Contour and Short Restorative Components.

Abutment Emergence Profile*	Color-coding
4.5 mmD	 Tan
5.5 mmD	 Rose
6.5 mmD	 Yellow

*For Hex-Lock Contour and Short Restorative components.

Hex-Lock Contour Abutments, Straight









Includes a Retaining Screw (MHLAS).

Implant Platform	Emergence Profile	Cuff Height		
		1.0 mm	2.0 mm	3.0 mm
 3.5 mmD	 4.5 mmD	ZOA341S	ZOA342S	ZOA343S
 4.5 mmD	 4.5 mmD	ZOA441S	ZOA442S	ZOA443S
 4.5 mmD	 5.5 mmD	ZOA451S	ZOA452S	ZOA453S
 5.7 mmD	 6.5 mmD	ZOA561S	ZOA562S	ZOA563S
Replacement Retaining Screw		MHLAS	MHLAS	MHLAS









Hex-Lock Contour Abutments, 17°

Includes a Retaining Screw (AH20S).

Implant Platform	Emergence Profile	Cuff Height	
		1.0 mm	2.0 mm
 3.5 mmD	 4.5 mmD	ZOA341A	ZOA342A
 4.5 mmD	 4.5 mmD	ZOA441A	ZOA442A
 4.5 mmD	 5.5 mmD	ZOA451A	ZOA452A
 5.7 mmD	 6.5 mmD	ZOA561A	ZOA562A
Replacement Retaining Screw		AH20S	AH20S



Contour Abutment Try-Ins and Try-In Kit

Implant Platform	Emergence Profile	Description	Item No.
 3.5 mmD	 4.5 mmD	Set of 5: Various Angles, Cuff Heights	ZOAT34
 4.5 mmD	 5.5 mmD	Set of 5: Various Angles, Cuff Heights	ZOAT45
 5.7 mmD	 6.5 mmD	Set of 5: Various Angles, Cuff Heights	ZOAT56
All	All	3 Sets of 5: All Sizes	ZOATKIT



Contour Provisional Copings

Emergence Profile	Straight	17°
● 4.5 mmD	ZCPROV4S	ZCPROV4A
● 5.5 mmD	ZCPROV5S	ZCPROV5A
● 6.5 mmD	ZCPROV6S	ZCPROV6A



Contour Impression Caps

Emergence Profile	Straight	17°
● 4.5 mmD	ZOCIMP4S	ZOCIMP4A
● 5.5 mmD	ZOCIMP5S	ZOCIMP5A
● 6.5 mmD	ZOCIMP6S	ZOCIMP6A



Contour Abutment Analogs, Titanium

Emergence Profile	Straight	Angled
● 4.5 mmD	TCANA4S	TCANA4A
● 5.5 mmD	TCANA5S	TCANA5A
● 6.5 mmD	TCANA6S	TCANA6A



Contour Waxing Copings

Emergence Profile	Straight	17°
● 4.5 mmD	ZOCWAX4S	ZOCWAX4A
● 5.5 mmD	ZOCWAX5S	ZOCWAX5A
● 6.5 mmD	ZOCWAX6S	ZOCWAX6A



Hex-Lock Short Abutments

Includes a Retaining Screw (MHLAS).

Implant Platform	Emergence Profile	Cuff Height	
		1.0 mm	2.0 mm
● 3.5 mmD	● 4.5 mmD	SA341	SA342
● 4.5 mmD	● 5.5 mmD	SA451	SA452
● 5.7 mmD	● 6.5 mmD	SA561	SA562
Replacement Retaining Screw		MHLAS	MHLAS



Short Provisional Copings

Emergence Profile	Item No.
● 4.5 mmD	SAPROVP4
● 5.5 mmD	SAPROVP5
● 6.5 mmD	SAPROVP6



Short Impression Caps

Emergence Profile	Item No.
● 4.5 mmD	SAIMP4
● 5.5 mmD	SAIMP5
● 6.5 mmD	SAIMP6



Short Abutment Analogs, Titanium

Emergence Profile	Item No.
● 4.5 mmD	SAANA4
● 5.5 mmD	SAANA5
● 6.5 mmD	SAANA6



Short Waxing Copings

Emergence Profile	Item No.
● 4.5 mmD	SAWAX4
● 5.5 mmD	SAWAX5
● 6.5 mmD	SAWAX6



Hex-Lock Abutments

Includes a Retaining Screw (MHLAS).

Implant Platform	Emergence Profile			
	3.5 mmD	4.5 mmD	5.5 mmD	6.5 mmD
● 3.5 mmD	HLA3/3	HLA3/4	HLA3/5	—
● 4.5 mmD	—	HLA4/4	HLA4/5	HLA4/6
● 5.7 mmD	—	—	—	HLA5/6
Replacement Retaining Screw, Short	MHLAS	MHLAS	MHLAS	MHLAS
Replacement Retaining Screw, Long	HLTS2	HLTS2	HLTS2	HLTS2



Angled Abutments, 20°, for 6 Positions

Two-piece abutment for 6 positions. Includes a Retaining Screw (AH20S).

Implant Platform	Emergence Profile	Item No.
● 3.5 mmD for 6 Positions	4.5 mmD	AH20/4
● 4.5 mmD for 6 Positions	5.5 mmD	AH20W/5
● 5.7 mmD for 6 Positions	6.5 mmD	A5H20/6
Replacement Retaining Screw	—	AH20S



Custom Abutments

GenTek Ti-Base Abutments*

Engaging*

Implant Platform	Cuff Height		
	0.3 mm	1.3 mm	2.6 mm
● 3.5 mmD	ZFX11ZB-TSV35AS03E	ZFX11ZB-TSV35AS13E	ZFX11ZB-TSV35AS26E
● 4.5 mmD	ZFX11ZB-TSV45AS03E	ZFX11ZB-TSV45AS13E	ZFX11ZB-TSV45AS26E
● 5.7 mmD	ZFX11ZB-TSV57AS03E	ZFX11ZB-TSV57AS13E	ZFX11ZB-TSV57AS26E



*Not available in all markets

Non-Engaging*


Implant Platform	Cuff Height	
	0.3 mm	1.3 mm
● 3.5 mmD	ZFX11ZB-TSV35AS03N	ZFX11ZB-TSV35AS13N
● 4.5 mmD	ZFX11ZB-TSV45AS03N	ZFX11ZB-TSV45AS13N
● 5.7 mmD	ZFX11ZB-TSV57AS03N	ZFX11ZB-TSV57AS13N



*Not available in all markets

Express and Flex Ti-Bases*

Implant Platform	Express		Flex	
	Hexed	Non-Hexed	Hexed	Non-Hexed
● 3.5 mmD	TE351	TE352	TF3121	TF3122
● 4.5 mmD	TE451	TE452	TF4121	TF4122
● 5.7 mmD	TE551	TE552	TF5121	TF5122

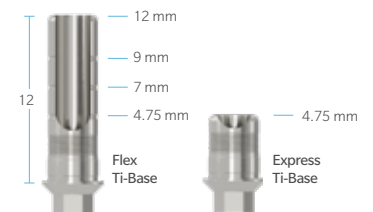

Includes ASC Screw (MHLASC).

*Not available in all markets

Patient-Specific BellaTek Abutments

Computer-aided design and custom-milled CAD/CAM precision.
Please contact a ZimVie Dental representative for additional information.

Note: Patient-Specific Abutments are only available in select markets.



"Cast-To" Gold Abutments, Engaging

Includes Retaining Screw (MHLAS).

Implant Platform	Item No.
● 3.5 mmD	HLA3G
● 4.5 mmD	HLA4G
● 5.7 mmD	HLA5G
Replacement Retaining Screw	MHLAS
Waxing Screw for "Cast-To" Abutments	MTWSD



"Cast-To" Gold Abutments, Non-Engaging

Includes Retaining Screw (MHLAS).

Implant Platform	Item No.
● 3.5 mmD	NEA3G
● 4.5 mmD	NEA4G
Replacement Retaining Screw	MHLAS



Screw-Retained Restorations

Straight Universal Multi-Unit Abutments

Non-engaging abutment does not engage in the internal hex connection. Not for use in single-unit restorations. Healing Cap (UMUA-HCS) sold separately.

Implant Platform	Collar Height				
	1.0 mm	2.0 mm	3.0 mm	4.0 mm	5.0 mm
● 3.5 mmD	UMUA-TSV351S	UMUA-TSV352S	UMUA-TSV353S	UMUA-TSV354S	UMUA-TSV355S
● 4.5 mmD	UMUA-TSV451S	UMUA-TSV452S	UMUA-TSV453S	UMUA-TSV454S	UMUA-TSV455S
● 5.7 mmD	UMUA-TSV571S	UMUA-TSV572S	UMUA-TSV573S	UMUA-TSV574S	UMUA-TSV575S



Angled Universal Multi-Unit Abutments, 17°

Abutments engage internal hex connection. Not for use in single unit (incl. preassembled retaining screw).

Implant Platform	Collar Height	
	2.5 mm	3.5 mm
● 3.5 mmD	UMUA-TSV3525-17S	UMUA-TSV3535-17S
● 4.5 mmD	UMUA-TSV4525-17S	UMUA-TSV4535-17S
● 5.7 mmD	UMUA-TSV5725-17S	UMUA-TSV5735-17S



Angled Universal Multi-Unit Abutments, 30°

Abutments engage internal hex connection. Not for use in single unit (incl. preassembled retaining screw).

Implant Platform	Collar Height	
	3.5 mm	4.5 mm
● 3.5 mmD	UMUA-TSV3535-30S	UMUA-TSV3545-30S
● 4.5 mmD	UMUA-TSV4535-30S	UMUA-TSV4545-30S
● 5.7 mmD	UMUA-TSV5735-30S	UMUA-TSV5745-30S



Components for Screw-Retained Restorations

Universal Abutments Healing Cap

Healing Cap threads onto the Universal Multi-Unit Abutment and Angled Multi-Unit Abutment.

Description	Item No.
Universal Abutments Healing Cap	UMUA-HCS



Universal Abutment Impression Coping

Impression Coping threads onto the Universal Multi-Unit Abutment and Angled Multi-Unit Abutment for impression-taking. This method transfers the abutment position.

Description	Height	Item No.
Universal Abutment Impression Coping, Open-Tray Includes Transfer Screws	—	UMUA-OTIC
Universal Abutment Impression Coping, Closed-Tray	5 mm	UMUA-CTICS
Universal Abutment Impression Coping, Closed-Tray, Qty 4	5 mm	UMUA-CTICS4
Universal Abutment Impression Coping, Closed-Tray	8 mm	UMUA-CTICL
Universal Abutment Impression Coping, Closed-Tray, Qty 4	8 mm	UMUA-CTICL4



Universal Abutment Scan Bodies

Scan Body threads onto the Universal Multi-Unit Abutment and Angled Multi-Unit Abutment.

Description	Item No.
Universal Abutment Scan Body, Intraoral	UMUA-SBIO
Universal Abutment Scan Body, Ti-Base, Qty 5	UMUA-SBTB5
Universal Abutment Scan Body, Desktop, Includes Multi-Unit Screw (UMUA-S)	UMUA-SBDT



Universal Abutment Ti-Base

Ti-Base threads onto the Universal Multi-Unit Abutment and Angled Multi-Unit Abutment.

Description	Height	Item No.
Universal Abutment Ti-Base, Includes Multi-Unit Screw (UMUA-S)	6 mm	UMUA-TTS
Universal Abutment Ti-Base, Includes Multi-Unit Screw (UMUA-S)	8 mm	UMUA-TTL



Universal Abutment Angulated Screw Channel Ti-Base

Description	Item No.
Universal Abutment Angulated Screw Channel Ti-Base Includes Angulated Screw Channel Screw (UMUA-ASCTS)	UMUA-ASCT



Universal Abutment Analog for Stone Models

Description	Item No.
Universal Abutment Analog	UMUA-A



Universal Abutment Digital Analog

Description	Item No.
Universal Abutment Digital Analog, Includes Screw	UMUA-DA



Universal Abutment Temporary Cylinder

Temporary Cylinder threads onto the Universal Multi-Unit Abutment and Angled Universal Multi-Unit Abutment.

Description	Item No.
Universal Abutment Temporary Cylinder, Includes Multi-Unit Screw (UMUA-S)	UMUA-TCS



Replacement Screws for Universal Multi-Unit Components

Description	Item No.
Universal Multi-Unit Screw	UMUA-S
Universal Angulated Screw Channel Screw	UMUA-ASCTS



Universal Abutment OverdenSURE® Attachment

Description	Item No.
Universal Abutment OverdenSURE Attachment	UMUA-ODS



Prosthetic Tools for Universal Multi-Unit Abutments

Description	Item No.
Universal Abutment Multi-Unit Driver	UMUA-D
ISO Latch, 4x4 Driver	ISO4X4A
Angulated Screw Channel Screwdriver, 24 mm(L)	ASC-SD24
Angulated Screw Channel Screwdriver, 30 mm(L)	ASC-SD30



Overdenture Attachments

OverdenSURE® Removable Attachment System Abutments (Available in the United States ONLY)

Seating Surface	Collar Height					
	1.0 mm	2.0 mm	3.0 mm	4.0 mm	5.0 mm	6.0 mm
● 3.5 mmD	ODSA-TSV301	ODSA-TSV302	ODSA-TSV303	ODSA-TSV304	ODSA-TSV305	ODSA-TSV306
● 4.5 mmD	ODSA-TSV401	ODSA-TSV402	ODSA-TSV403	ODSA-TSV404	ODSA-TSV405	ODSA-TSV406
● 5.7 mmD	ODSA-TSV501	ODSA-TSV502	ODSA-TSV503	ODSA-TSV504	ODSA-TSV505	ODSA-TSV506



Retention Kit ODSZ-RIKIT2001 not included, please order separately.

(Available outside the United States ONLY)

Seating Surface	Collar Height					
	1.0 mm	2.0 mm	3.0 mm	4.0 mm	5.0 mm	6.0 mm
● 3.5 mmD	ODS-TSV301	ODS-TSV302	ODS-TSV303	ODS-TSV304	ODS-TSV305	ODS-TSV306
● 4.5 mmD	ODS-TSV401	ODS-TSV402	ODS-TSV403	ODS-TSV404	ODS-TSV405	ODS-TSV406
● 5.7 mmD	ODS-TSV501	ODS-TSV502	ODS-TSV503	ODS-TSV504	ODS-TSV505	ODS-TSV506



Retention Kit ODS-RIKIT2001 included. Available in all active geographies except the U.S.

OverdenSURE Retention Inserts

Description	Item No.
Retention Kit 20° Qty 1 Set	ODSZ-RIKIT2001
Retention Kit 20° Qty 2 Sets	ODSZ-RIKIT2002
Retention Kit 40° Qty 1 Set	ODSZ-RIKIT4001
Retention Kit 40° Qty 2 Sets	ODSZ-RIKIT4002
Blue Retention Insert 20° Qty 4	ODSZ-RIB2004
Pink Retention Insert 20° Qty 4	ODSZ-RIP2004
Clear Retention Insert 20° Qty 4	ODSZ-RIC2004
Red Retention Insert 40° Qty 4	ODSZ-RIR4004
Yellow Retention Insert 40° Qty 4	ODSZ-RIY4004
Green Retention Insert 40° Qty 4	ODSZ-RIG4004



U.S. market only.

OverdenSURE Accessories

Description	Item No.
Abutment Bar Attachment Qty 1	ODS-BARATT01
Abutment Bar Attachment Qty 2	ODS-BARATT02
Abutment Bar Attachment Qty 4	ODS-BARATT04
Analog Qty 1	ODS-AA01
Analog Qty 4	ODS-AA04
Analog Qty 10	ODS-AA010
Blockout Spacer Qty 20	ODS-BS020
Impression Coping Qty 1	ODS-IC01
Impression Coping Qty 4	ODS-IC04
Impression Coping Qty 10	ODS-IC010
Retention Housing Cap Qty 1	ODS-RH01
Retention Housing Cap Qty 4	ODS-RH04
Retention Housing Cap Qty 10	ODS-RH010
Scan Body Qty 10	ODS-SB010



OverdenSURE Attachment Components

Description	Item No.
Retention Kit 20° Qty 1 Set	ODS-RIKIT2001
Retention Kit 20° Qty 2 Sets	ODS-RIKIT2002
Retention Kit 40° Qty 1 Set	ODS-RIKIT4001
Retention Kit 40° Qty 2 Sets	ODS-RIKIT4002
Blue Retention Insert 20° Qty 4	ODS-RIB2004
Pink Retention Insert 20° Qty 4	ODS-RIP2004
Clear Retention Insert 20° Qty 4	ODS-RIC2004
Red Retention Insert 40° Qty 4	ODS-RIR4004
Yellow Retention Insert 40° Qty 4	ODS-RIY4004
Green Retention Insert 40° Qty 4	ODS-RIG4004



All markets outside U.S.

Ball Abutments

Abutments do not engage internal hex connection. Includes Cap Attachment Housing and Nylon Liner.

Implant Platform	Cuff Height		
	2.0 mm	4.0 mm	6.0 mm
● 3.5 mmD	BAC2	BAC4	BAC6
● 4.5 mmD	BACW2	BACW4	BACW6
● 5.7 mmD	BA5C2	BA5C4	—



Ball Abutment Transfer Components


Description	Item No.
Ball Abutment Transfer (Qty. 2)	BAT
Ball Abutment Replica	BAR



Prosthetic Tools

Prosthetic Components

Description	Item No.
Cap Attachment System Includes 4 Nylon Liners, 2 Positioning Rings, 4 Housings, and 4 Castable Ball Patterns	CAS
Cap Attachment Instruments Includes Seating Tool, Reamer, and Paralleling Tool	CAI
Cap Attachment Housing (CAH)/Cap Attachment Nylon Liner (CAN)	CA
Cap Attachment Housing	CAH
Cap Attachment Nylon Liner, Transparent	CAN
Cap Attachment Nylon Liner, Gray — Rigid Retention	CAN-G
Cap Attachment Transfer	CAT
Castable Ball Pattern, 2 balls per pattern	CAB
Micro Cap Attachment Nylon Liner	CANM




Angled Screw Channel Tools for GenTek Abutments

Description	Mode of Use	Item No.
Angled Screw Channel Driver 24 mmL	TWR	TASCD24
Angled Screw Channel Driver 30 mmL	TWR	TASCD30
Angled Screw Channel Driver Tip 21 mmL	L-TIRW	ZFX02HLD21
Angled Screw Channel Driver Tip 24 mmL	L-TIRW	TASCT24
Angled Screw Channel Driver Tip 28 mmL	L-TIRW	ZFX02HLD28
Angled Screw Channel Driver Tip 30 mmL	L-TIRW	TASCT30
Angled Screw Channel Driver Tip 36 mmL	L-TIRW	ZFX02HLD36



Angled Screw Channel Tools for Express and Flex Abutments

Description	Mode of Use	Item No.
Angled Screw Channel Driver, 24 mmL	TWR	TASCD24
Angled Screw Channel Driver, 30 mmL	TWR	TASCD30
Angled Screw Channel Driver Tip, 24 mmL	L-TIRW	TASCT24
Angled Screw Channel Driver Tip, 30 mmL	L-TIRW	TASCT30




Additional Prosthetic Tools

Description	Item No.
Hex Driver, Short, with GemLock® Retention, 1.25 mmD, 22 mmL	HXGR1.25
Hex Driver, Long, with GemLock Retention, 1.25 mmD, 30 mmL	HXLGR1.25
Hex Driver, Short, Standard, 1.25 mmD, 17 mmL	HX1.25
Hex Driver, Long, Standard, 1.25 mmD, 22 mmL	HXL1.25
Latch-Lock Hex Driver for Surgical and Prosthetic Screws, Short, 1.25 mmD, 23 mmL May require Reduction Handpiece	HX1.25D
Latch-Lock Hex-Driver for Surgical and Prosthetic Screws, Long, 1.25 mmD, 26 mmL May require Reduction Handpiece	HXL1.25D
Torque Wrench, Restorative Adjustable torque range 10 Ncm – 35 Ncm	TWR
Torque Wrench Hex Driver, Short, 1.25 mmD, 17 mmL	TW1.25
Torque Wrench Hex Driver, Long, 1.25 mmD, 22 mmL	TW1.25L
Removal and Insertion Tool	ODS-IRTOOL
Prosthetic Kit Tray, Autoclavable, empty	2320
Removal Tool for Internal Hex Implant Abutments Included in TSV Surgical Kits TSVKIT and STRKIT	TLRT2
Removal Screw for Internal Hex Implant Abutments	HLRS
Abutment Holder Requires Implant Analog to attach abutments	ABTH
Removal Tool for Abutment Screws or Fixation Screws with 1.25 mmD Hex, Carbide Steel Note: Do not autoclave	SRT




Instrument Kit System

Instrument Kit System Overview TSV Surgical Kit (TSVKIT)

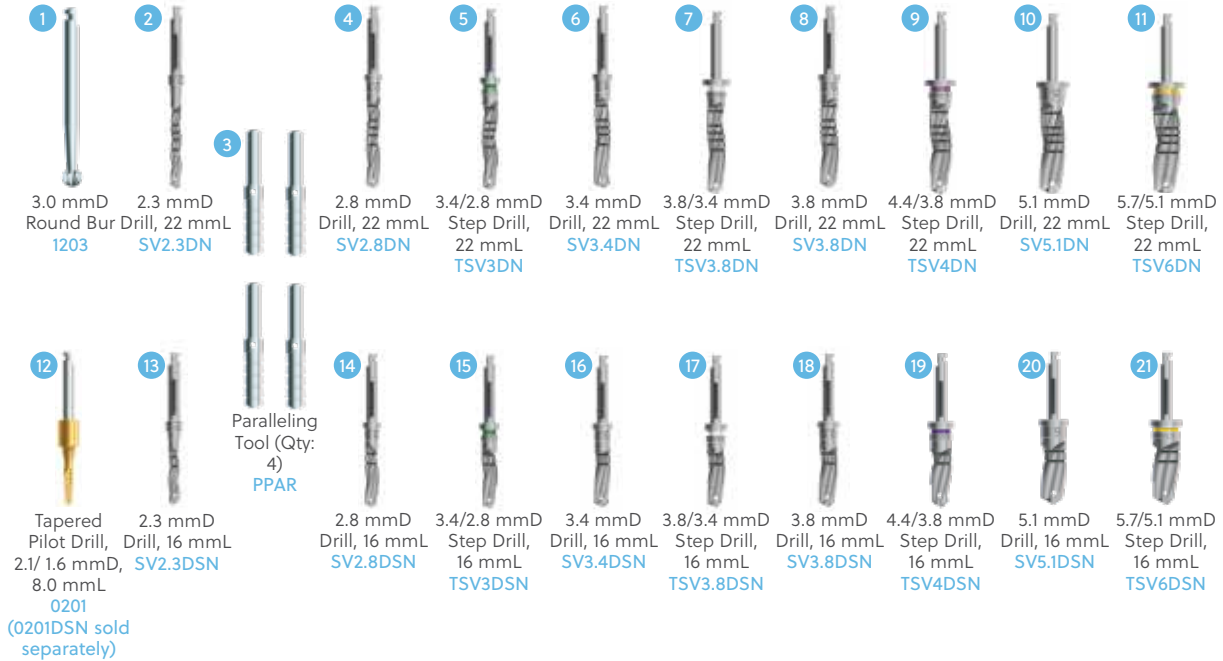




Guided Surgery Drill Module (GSMOD)

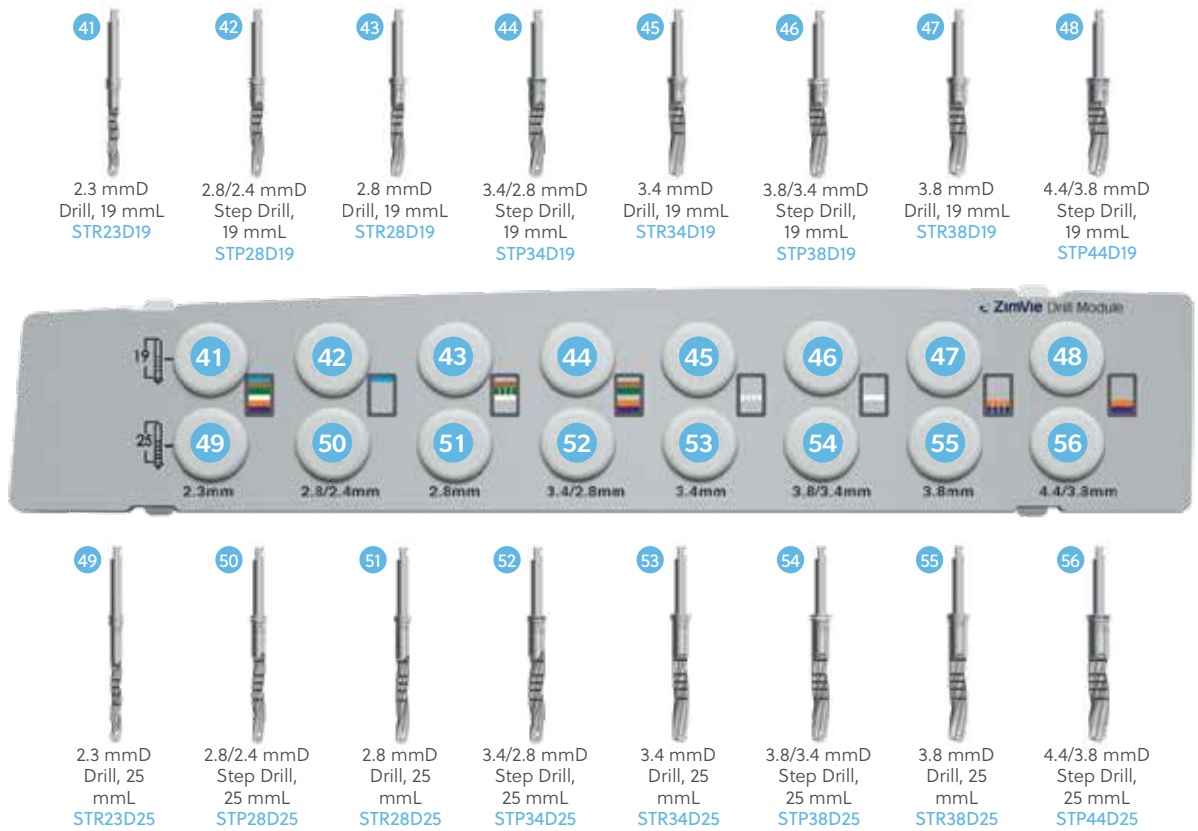

The NP Surgical Module snaps into the TSV Surgical Kit

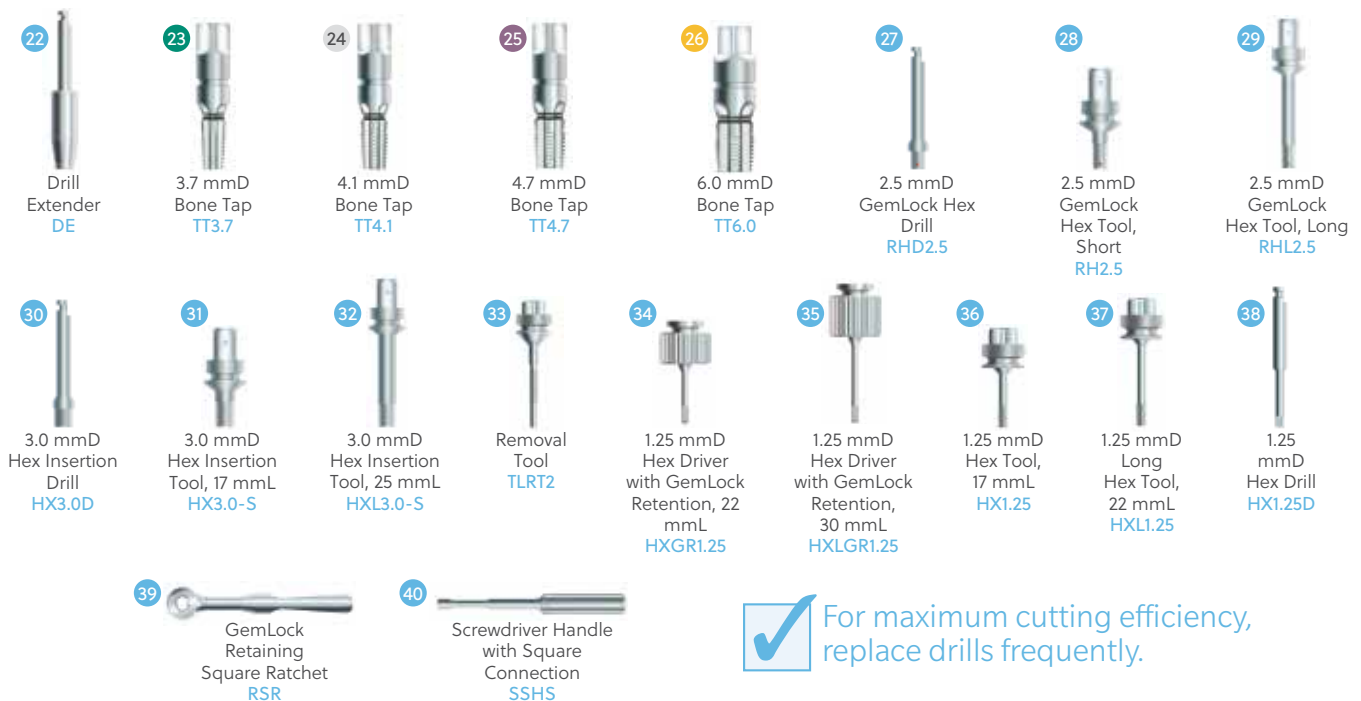

 For maximum cutting efficiency, replace drills frequently.

TSV Surgical Kit

TSV Surgical Kit, Complete

Description	Item No.
TSV Surgical Kit For placement of 3.7 mmD, 4.1 mmD, 4.7 mmD, and 6.0 mmD TSV and TM Implants	TSVKIT
TSV Surgical Tray, Empty	TSVTRAY
2.1/1.6 mmD Drill, 8 mmL	0201
Round Bur	1203
2.3 mmD Dríva™ Surgical Drill, 16 mmL	SV2.3DSN
2.3 mmD Dríva Surgical Drill, 22 mmL	SV2.3DN
2.8 mmD Dríva Surgical Drill, 16 mmL	SV2.8DSN
2.8 mmD Dríva Surgical Drill, 22 mmL	SV2.8DN
3.4/2.8 mmD Dríva Surgical Step Drill, 16 mmL	TSV3DSN
3.4/2.8 mmD Dríva Surgical Step Drill, 22 mmL	TSV3DN
3.4 mmD Dríva Surgical Drill, 16 mmL	SV3.4DSN
3.4 mmD Dríva Surgical Drill, 22 mmL	SV3.4DN
3.8/3.4 mmD Dríva Surgical Step Drill, 16 mmL	TSV3.8DSN
3.8/3.4 mmD Dríva Surgical Step Drill, 22 mmL	TSV3.8DN
3.8 mmD Dríva Surgical Drill, 16 mmL	SV3.8DSN
3.8 mmD Dríva Surgical Drill, 22 mmL	SV3.8DN
4.4/3.8 mmD Dríva Surgical Step Drill, 16 mmL	TSV4DSN
4.4/3.8 mmD Dríva Surgical Step Drill, 22 mmL	TSV4DN
5.1 mmD Dríva Surgical Drill, 16 mmL	SV5.1DSN
5.1 mmD Dríva Surgical Drill, 22 mmL	SV5.1DN
5.7/5.1 mmD Dríva Surgical Step Drill, 16 mmL	TSV6DSN
5.7/5.1 mmD Dríva Surgical Step Drill, 22 mmL	TSV6DN
3.7 mmD Cortical Bone Tap Tool	TT3.7
4.1 mmD Cortical Bone Tap Tool	TT4.1
4.7 mmD Cortical Bone Tap Tool	TT4.7
6.0 mmD Cortical Bone Tap Tool	TT6.0
1.25 mmD Hex Driver, Short, with GemLock Retention, 22 mmL	HXGR1.25
1.25 mmD Hex Driver, Long, with GemLock Retention, 30 mmL	HXLGR1.25
1.25 mmD Hex Driver, Short, 17 mmL	HX1.25
1.25 mmD Hex Driver, Long, 22 mmL	HXL1.25
1.25 mmD Latch-Lock Hex Driver, 23 mmL	HX1.25D
2.5 mmD GemLock Retaining Hex Driver, Short, 17 mmL	RH2.5
2.5 mmD GemLock Retaining Hex Driver, Long, 28 mmL	RHL2.5
2.5 mmD GemLock Retaining Hex Driver, 21 mmL	RHD2.5
3.0 mmD Hex Driver, Short, 17 mmL*	HX3.0-S
3.0 mmD Hex Driver, Long, 28 mmL*	HXL3.0-S
3.0 mmD Hex Driver, 25 mmL*	HX3.0D
Drill Extender, 27 mmL	DE
Paralleling Tool (Qty. 4)	PPAR
GemLock Retaining Square Ratchet	RSR
Screwdriver Handle with Square Connection	SSHS
Removal Tool for Internal Hex Implant Abutments	TLRT2
TSV Staging Block	TSVBLK



Note: Drills marked in blue are included in TSVTRAYD on page 25.

*3.0 mmD Hex Drivers engage the internal hex of the 6.0 mmD implants when the Fixture Mount/Transfer is removed.

TSV Surgical Kit, Partial Configurations

Description	Item No.
TSV Starter Kit For placement of 3.7 mmD and 4.7 mmD Implants only	STRKIT
2.1/1.6 mmD Drill, 8 mmL	0201
2.3 mmD Dríva Surgical Drill, Instrument Kit System, 22 mmL	SV2.3DN
2.8 mmD Dríva Surgical Drill, Instrument Kit System, 22 mmL	SV2.8DN
3.4/2.8 mmD Dríva Surgical Step Drill, Instrument Kit System, 22 mmL	TSV3DN
3.8 mmD Dríva Surgical Drill, Instrument Kit System, 22 mmL	SV3.8DN
4.4/3.8 mmD Dríva Surgical Step Drill, Instrument Kit System, 22 mmL	TSV4DN
1.25 mmD Hex Driver, Short, with GemLock Retention, 22 mmL	HXGR1.25
1.25 mmD Hex Driver, Long, with GemLock Retention, 30 mmL	HXLGR1.25
1.25 mmD Hex Driver, Short, 17 mmL	HX1.25
2.5 mmD GemLock Retaining Hex Driver, Long, 28 mmL	RHL2.5
2.5 mmD GemLock Retaining Hex Driver, 21 mmL	RHD2.5
Drill Extender, 27 mmL	DE
Paralleling Tool (Qty. 4)	PPAR
GemLock Retaining Square Ratchet	RSR
Screwdriver Handle with Square Connection	SSHS
Removal Tool for Internal Hex Implant Abutments	TLRT2
3.7 mmD Cortical Bone Tap Tool	TT3.7
4.7 mmD Cortical Bone Tap Tool	TT4.7
TSV Staging Block	TSVBLK
TSV Surgical Tray, Empty	TSVTRAY
Surgical Tray and Drills for TM and TSV Implants Includes TSVBLK and drills marked in blue on page 24 ; Tray and drills only	TSVTRAYD
Tapered Screw-Vent Staging Block Block only	TSVBLK



Guided Surgery Instrumentation

Description	Item No.
Guided Surgery Drill Module Can be inserted into the TSVKIT for an all-in-one Guided Surgery Kit	GSMOD
2.3 mmD Dríva EG Surgical Drill, 19 mmL	STR23D19
2.3 mmD Dríva EG Surgical Drill, 25 mmL	STR23D25
2.8/2.4 mmD Dríva EG Surgical Step Drill, 19 mmL	STP28D19
2.8/2.4 mmD Dríva EG Surgical Step Drill, 25 mmL	STP28D25
2.8 mmD Dríva EG Surgical Drill, 19 mmL	STR28D19
2.8 mmD Dríva EG Surgical Drill, 25 mmL	STR28D25
3.4/2.8 mmD Dríva EG Surgical Step Drill, 19 mmL	STP34D19
3.4/2.8 mmD Dríva EG Surgical Step Drill, 25 mmL	STP34D25
3.4 mmD Dríva EG Surgical Drill, 19 mmL	STR34D19
3.4 mmD Dríva EG Surgical Drill, 25 mmL	STR34D25
3.8/3.4 mmD Dríva EG Surgical Step Drill, 19 mmL	STP38D19
3.8/3.4 mmD Dríva EG Surgical Step Drill, 25 mmL	STP38D25
3.8 mmD Dríva EG Surgical Drill, 19 mmL	STR38D19
3.8 mmD Dríva EG Surgical Drill, 25 mmL	STR38D25
4.4/3.8 mmD Dríva EG Surgical Step Drill, 19 mmL	STP44D19
4.4/3.8 mmD Dríva EG Surgical Step Drill, 25 mmL	STP44D25



Guided Surgery Module Insert (Empty)	GSTRAY
--------------------------------------	--------



Tube Adapter Kit* Includes 1 of each Tube Adapter listed below; EG Drills are used with Tube Adapter Kit;	TADKIT
2.3 mmD Tube Adapter, A	TAD23A
2.8 mmD Tube Adapter, A	TAD28A
3.4 mmD Tube Adapter, A	TAD34A
2.3 mmD Tube Adapter, B	TAD23B
2.8 mmD Tube Adapter, B	TAD28B
3.4 mmD Tube Adapter, B	TAD34B
3.8 mmD Tube Adapter, B	TAD38B
4.4 mmD Tube Adapter, B	TAD44B




*Must use drills with axial stripe.

Dríva Surgical Drills

A product of extensive research and testing, high performance and internally-irrigated Dríva Drills are reusable and deliver high levels of sharpness and longevity.

- Enhanced drill design to facilitate cleaning and sterilization
- Color bands and size etching help in simple identification and replacement
- All drills are made of an advanced grade of stainless steel, with a progressive geometry that provides high levels of strength and cutting efficiency
- A corrosion-resistant coating protects drill sharpness
- Grooves and laser-etched depth bands deliver improved visibility

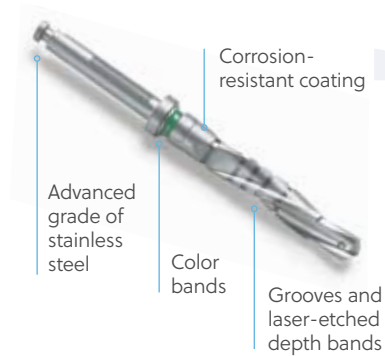

Surgical Pilot Drills

Diameter	8.0 mmL	15 mmL*	16 mmL*	19 mmL	22 mmL*	25 mmL
2.1/1.6 mmD	—	0201DSN	—	—	—	—
2.1/1.6 mmD	0201	—	—	—	—	—



Dríva Surgical Drills

Diameter	8.0 mmL	15 mmL*	16 mmL*	19 mmL	22 mmL*	25 mmL
2.3 mmD	—	—	SV2.3DSN	STR23D19	SV2.3DN	STR23D25
2.8 mmD	—	—	SV2.8DSN	STR28D19	SV2.8DN	STR28D25
3.4 mmD	—	—	SV3.4DSN	STR34D19	SV3.4DN	STR34D25
3.8 mmD	—	—	SV3.8DSN	STR38D19	SV3.8DN	STR38D25
5.1 mmD	—	—	SV5.1DSN	—	SV5.1DN	—




Dríva Surgical Step Drills

Diameter	16 mmL*	19 mmL	22 mmL*	25 mmL	Color Code
2.8/2.4 mmD	—	STP28D19	ZOP28DN	STP28D25	Blue
3.4/2.8 mmD	TSV3DSN	STP34D19	TSV3DN	STP34D25	Green
3.8/3.4 mmD	TSV3.8DSN	STP38D19	TSV3.8DN	STP38D25	White
4.4/3.8 mmD	TSV4DSN	STP44D19	TSV4DN	STP44D25	Purple
5.1/4.4 mmD	TSV5.1DSN **	—	TSV5.1DN **	—	—
5.7/5.1 mmD	TSV6DSN	—	TSV6DN	—	Yellow



*The 15 mmL, 16 mmL and 22 mmL Drills feature axial stripes to help identify use with the Drill Stop Kit.

**TSV5.1DSN and TSV5.1DN are interim drills sold separately and not in surgical kits.

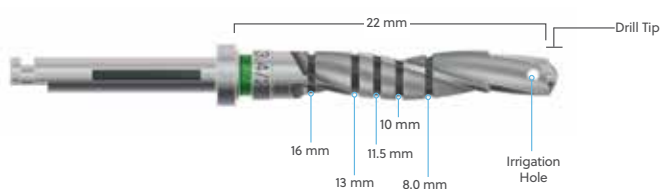

The depth markings are machined and laser-etched for increased visibility.

The bands are located approximately 1.0 mm longer than the implant-abutment junction. (for example: the 13 mm band is dimensioned 14 mm from the tip of the drill)

Instrumentation

Cleaning Tool

Description	Item No.	Qty.
Dríva Drill Cleaning Wire	NM1940	1 Ea.



Implant Placement Instruments

Description	Item No.
GemLock Retaining Square Ratchet for Implant Placement with Hex Drivers RH2.5/RHL2.5 or FMT Directly	RSR
Stainless Steel Screwdriver Handle with Square Connection for Implant Placement with Hex Drivers RH2.5/RHL2.5 or FMT Directly	SSHS



Hex Drivers 1.25 mmD

Description	Item No.
Hex Driver, Short, for Tightening of Surgical and Prosthetic Screws, 17 mmL	HX1.25
Hex Driver, Long, for Tightening of Surgical and Prosthetic Screws, 22 mmL	HXL1.25
Hex Driver, Short, with GemLock Retention, 22 mmL	HXGR1.25
Hex Driver, Long, with GemLock Retention, 30 mmL	HXLGR1.25
Latch-Lock Hex Driver for Surgical and Prosthetic Screws, Short, 23 mmL May require Reduction Handpiece	HX1.25D
Latch-Lock Hex Driver for Surgical and Prosthetic Screws, Long, 26 mmL May require Reduction Handpiece	HXL1.25D



Hex Drivers 2.5 mmD


Description	Item No.
GemLock Retaining Hex Driver, 21 mmL	RHD2.5
GemLock Retaining Hex Driver, Short, 17 mmL	RH2.5
GemLock Retaining Hex Driver, Long, 28 mmL	RHL2.5



Note: 2.5 mmD Hex Drivers (GemLock Delivery System) should be used to deliver all TSV Implants via the Fixture Mount/Transfer.

Hex Drivers 3.0 mmD

Description	Item No.
Hex Driver for Implants with 3.0 mmD Hex, 25 mmL May require Reduction Handpiece	HX3.0D
Hex Driver, Short, for Implants with 3.0 mmD Hex, 17 mmL	HX3.0-S
Hex Driver, Long, for Implants with 3.0 mmD Hex, 28 mmL	HXL3.0-S



Note: 3.0 mmD Hex Drivers are used to place the 6.0 mmD TSV Implants without a Fixture Mount/Transfer.

Cortical Bone Taps (Triple-Lead Threads)

Description	Item No.
3.7 mmD Cortical Bone Tap Tool	TT3.7
4.1 mmD Cortical Bone Tap Tool	TT4.1
4.7 mmD Cortical Bone Tap Tool	TT4.7
6.0 mmD Cortical Bone Tap Tool	TT6.0



Surgical Instruments

Description	Item No.
Drill Extender, 27 mmL	DE
Paralleling Tool	PPAR
Removal Tool for Screw-Type Implants, Carbide Steel Note: Do not autoclave	IRT
Removal Tool for Internal Hex Implant Abutments Included in TSV Surgical Kits TSVKIT and STRKIT	TLRT2
Round Bur	1203
Manual Interchangeable Driver Tip Handle	MIDTH



Drill Stop Kit

Single-Patient Drills

Description	Contents	Item No.
Drill Kit, Single-Patient, Long 3.7 mmD Implant, 17 mmL	3.0 mmD Round Bur 2.3 mmD Pilot Drill 3.4/2.8 mmD Step Drill	DSTK3
Drill Kit, Single-Patient, Short 3.7 mmD Implant, 11 mmL	3.0 mmD Round Bur 2.3 mmD Pilot Drill 3.4/2.8 mmD Step Drill	DSTK3S
Drill, Single-Patient, Long 4.7 mmD Implant, 17 mmL	4.4/3.8 mmD Step Drill	DST4
Drill, Single-Patient, Short 4.7 mmD Implant, 11 mmL	4.4/3.8 mmD Step Drill	DST4S
Drill, Single-Patient, Long 6.0 mmD Implant, 17 mmL	5.7/5.1 mmD Step Drill	DST6
Drill, Single-Patient, Short 6.0 mmD Implant, 11 mmL	5.7/5.1 mmD Step Drill	DST6S

Note: No internal irrigation. Kits with long drills have depth markings for 8, 10, 11.5, 13, and 16 mmL implants. Kits with short drills have depth markings for 8 and 10 mmL implants.

Radiographic Transparency

Description	Item No.
Radiographic Transparency for TSV	RT-TSV

Drill Stop Kit

Description	Item No.
Complete Drill Stop Kit <i>Drills not included</i>	DSKIT
Stop Set, 8.0 mmL Implant, 2.3 - 4.4/3.8 mmD x 17/22 mmL Dríva Drill (Qty. 5)	SS8D22
Stop Set, 10 mmL Implant, 2.3 - 4.4/3.8 mmD x 17/22 mmL Dríva Drill (Qty. 5)	SS10D22
Stop Set, 11.5 mmL Implant, 2.3 - 4.4/3.8 mmD x 17/22 mmL Dríva Drill (Qty. 5)	SS11D22
Stop Set, 13 mmL Implant, 2.3 - 4.4/3.8 mmD x 17/22 mmL Dríva Drill (Qty. 5)	SS13D22
Stop Set, 8 mmL Implant, 2.3 - 4.4/3.8 mmD x 11/16 mmL Dríva Drill (Qty. 5)	SS8D16
Stop Set, 10 mmL Implant - 11/16 mmL Dríva Drill and 16 mmL Implant - 17/22 mmL Dríva Drill, 2.3 - 4.4/3.8 mmD Dríva Drill (Qty. 5)	SS10D16
Stop Set, 11.5 mmL Implant, 2.3 - 4.4/3.8 mmD x 11/16 mmL Dríva Drill (Qty. 5)	SS11D16
Stop Set, 8-16 mmL Implant, 5.1 mmD x 11/16 mmL & 17/22 mmL Dríva Drill (Qty. 7)	SS51D
Stop Set, 8-16 mmL Implant, 5.7/5.1 mmD x 11/16 mmL & 17/22 mmL Dríva Drill (Qty. 7)	SS57D
Drill Stop Multi-Tool	MTL



For more information, visit ZimVie.com

ZimVie US Corp LLC
4555 Riverside Drive
Palm Beach Gardens, FL 33410
Phone: +1-561-776-6700
Fax: +1-561-776-1272
dentalCS@ZimVie.com



Unless otherwise indicated, as referenced herein, all trademarks and intellectual property rights are the property of ZimVie Inc. and its affiliates; and all products are manufactured by one or more of the dental subsidiaries of ZimVie US Corp LLC (Biomet 3i, LLC, etc.) and distributed by ZimVie US Corp LLC and its authorized marketing partners. OverdenSURE is manufactured by Terrats Medical S.L. EU Medical device classification: Dental Implant (Class IIb); Dental Surgical Instruments (Class IIb); Definitive Abutments (Class IIb); Provisional Copings, Healing Caps and Restorative Components (Class I). The Intended purpose of Dental Implants is to replace missing individual teeth (single tooth restorations), multiple teeth, or edentulous dental arches (implant retained fixed bridge, implant-supported overdenture) by providing a means for prosthetic attachment. The intended purpose of the Healing Screw and Surgical Cover Screws is to seal the implant internal connection and separate it from the soft tissue which is sutured over the implant during the healing process. The intended purpose of fixture mount/transfers is primarily to facilitate the delivery, appropriate alignment, positioning, and placement of the associated implants. When used as a provisional abutment, fixture mount/transfers are intended for use in conjunction with endosseous dental implants for placement in the maxilla and mandible for up to 180 days during endosseous and gingival healing to prepare gingival tissue for acceptance of a final abutment and restoration. Dental Instruments are intended to facilitate the implantation and explantation of the corresponding Dental Implants, and for use in conjunction with dental restorative devices and processes. Definitive Abutments are intended for use in conjunction with endosseous dental implants for placement in the maxilla and mandible to support a permanent restoration. Provisional Copings are intended for use in conjunction with definitive abutments for up to 180 days during endosseous and gingival healing to support a provisional restoration. Healing Caps protect the abutment surface and threaded opening from the surrounding oral environment prior to completion of the restoration. Restorative Components (e.g., Impression Cap, Abutment Try-In) are intended to facilitate the positional reference of an abutment. Some Restorative Components (e.g., Abutment Analog, Waxing Coping) are intended for the fabrication of a restoration. The products here shown are not eligible for reimbursement in France. For other countries, please check the local laws and regulation. For additional product information, please refer to the individual product labeling or instructions for use. Product clearance and availability may be limited to certain countries/regions. This material is intended for clinicians only and does not comprise medical advice or recommendations. Distribution to any other recipient is prohibited. This material may not be copied or reprinted without the express written consent of ZimVie and is not for distribution in France. ZVINST0151-GLBL REV B 04/26 ©2026 ZimVie. All rights reserved.

